



Instruction Manual

Nova-Pro® Ultraviolet UV365 and UV385 LED Stroboscopes/Laser Tachometers



PATENTED
TECHNOLOGY



NIST
CALIBRATION



15 Columbia Drive, Amherst, NH 03031 USA

Phone: (603) 883-3390 • Fax: (603) 886-3300

E-mail: support@monarchinstrument.com

Website: www.monarchinstrument.com



SAFEGUARDS AND PRECAUTIONS



1. Read and follow all instructions in this manual carefully, and retain this manual for future reference.
2. Do not use this instrument in any manner inconsistent with these operating instructions or under any conditions that exceed the environmental specifications stated.
3. Certain strobe frequencies can trigger epileptic seizures in those prone to that type of attack.



4. **CAUTION: UV emitted from this product. Eye or skin irritation may result from exposure. Use appropriate shielding. DO NOT STARE AT THE LIGHT SOURCE.**

5. Exposure to flickering light or visual patterns may cause eye strain, headaches, nausea, dizziness, and other afflictions.
6. Objects viewed with this product may appear to be stationary when in fact they are moving at high speeds. Always keep a safe distance from moving machinery and do not touch the target.
7. There are no user serviceable parts in this instrument. Refer service to a qualified technician.
8. This instrument may not be safe for use in certain hazardous environments, and serious personal injury or death could occur as a result of improper use. Please refer to your facility's safety program for proper precautions.
9. Do not clean this instrument with alcohol or other cleaning solvents as these may damage the LEDs.




To comply with worldwide regulations such as the U.S. Environmental Protection Agency Resource Conservation and Recovery Act (RCRA) and EU Directive 2012/19/EU on Waste Electrical and Electronic Equipment (WEEE), you must not discard this electrical/electronic product in domestic household waste. The electronic components in this device may contain environmentally harmful substances. DO NOT DISPOSE of this product as unsorted municipal waste. This product needs to be RECYCLED and disposed of in accordance with environmental regulations in the country of use; contact your local authorities for more information. This product may be returnable to your distributor for recycling; contact the distributor for details.



Nova-Pro Battery Packs contain Lithium-ion batteries which must be recycled and disposed of in accordance with Federal, State, & Local Regulations. Do not incinerate. Batteries should be shipped to a reclamation facility for recovery of the metal and plastic components as the proper method of waste management. Contact the distributor for appropriate product return procedures.

LASER MODULE



Diode Laser

Max. Output Power: **<1 milliwatt**
Wavelength: **650 nanometers (visible light)**
Beam Divergence: **<18 milliradian**
Output: **Continuous (CW)**
Laser Hazard Classification: **Class 2**

Laser Hazards:

Eye injury from beam - Do not look into the direct or reflected beam; can cause eye injury up to 25 ft. [7.5 m] away.

Visual interference (glare) with pilots and drivers - Interferes with vision up to 525 ft (160 m) away. Can be a distraction up to 1 mile [1.6 km] away. ***NEVER point any laser towards aircraft or vehicles; it is unsafe and illegal.***

Safe Use Guidance:

Class 2 lasers are considered safe for accidental eye exposure. Do not look or stare into beam. Do not aim at aircraft. ***This is not a toy.*** Always supervise children.

Manufacturer:

Monarch Instrument
15 Columbia Drive
Amherst, NH 03031 USA
Country of Origin: USA
Contact info: www.monarchinstrument.com

Monarch Instrument's Limited Warranty applies.
See www.monarchinstrument.com for details.

Warranty Registration and Extended Warranty Coverage information is available online at www.monarchinstrument.com.

Monarch Instrument holds the following US trademarks and registrations, all rights reserved: illumiNova®, Nova-Pro®, Nova-Strobe™, DataChart™, Track-It™.
This product is protected by United States Patent No. 10,080,268.

TABLE OF CONTENTS:

1.0 INTRODUCTION.....	1
2.0 USER INTERFACE	3
3.0 GETTING STARTED.....	5
3.1 Power	5
3.1.1 Continuous Operation.....	5
3.2 Input/Output Connections.....	6
4.0 MODES OF OPERATION	7
4.1 STROBE Mode.....	7
4.1.1 Joystick	7
4.1.2 Touch Keypad Entry.....	8
4.1.3 Doubling or Halving the Flash Rate.....	8
4.1.4 External Input.....	9
4.2 LAMP Mode.....	10
4.3 LASER Mode	10
4.4 TACH (Tachometer) Mode	12
5.0 MENUS	13
5.1 Menu Overview	14
5.2 MODE Menu	15
5.3 Brightness (BRITE) Menu.....	15
5.3.1 Degrees	16
5.3.2 Time	16
5.4 Miscellaneous (MISC) Menu.....	17
5.4.1 DECPT (Decimal Point) Menu	17
5.4.2 UNITS Menu.....	18
5.4.3 INPUT Menu	18
5.4.4 OUTP (OUTPUT) Menu	19
5.4.5 BKLIT (Backlight) Menu	19
5.5 Memory (MEMRY) Menu	19
5.5.1 Save Memory.....	20
5.5.2 Recall Memory.....	20

5.6 JOG Menu	21
5.6.1 NONE.....	21
5.6.2 PHASE.....	21
5.6.3 TIME	21
5.7 DELAY Menu	22
5.7.1 NONE.....	23
5.7.2 PHASE.....	23
5.7.3 TIME	23
5.7.4 VRPM	23
6.0 STROBE BRIGHTNESS	24
6.1 Calculating Blur.....	24
6.2 Brightness in Degrees of Rotation	25
6.3 Brightness in Pulse Duration	25
7.0 STROBE DELAY	26
7.1 Internal Phase Delay (JOG).....	26
7.2 External / Laser Delay	27
7.2.1 Phase Delay	27
7.2.2 Time Delay.....	28
7.2.3 AUTO—Virtual RPM.....	28
8.0 BATTERY PACK	29
8.1 Low Battery Functionality	29
8.2 Charging the Battery Pack	30
9.0 OPTIONAL AC POWER	31
10.0 WALL POWER SUPPLIES	31
11.0 SPECIFICATIONS	32
11.1 Operating Environment.....	33
11.2 Compliance.....	33
11.2.1 Battery Compliance.....	33
11.2.2 EU Declaration of Conformity.....	34
11.2.3 Energy Efficiency	34
12.0 ACCESSORIES.....	34

1.0 INTRODUCTION

The Nova-Pro® UV365/385 are portable handheld UV LED Stroboscope/Lamps used for inspection and to stop motion of moving objects. They emit UVA light at 365nm or 385nm respectively. They come standard as battery powered and have delay functions which enable the user to delay the flash by degrees or time and do virtual slow motion inspection of rotating and reciprocating objects. Both models have a dedicated Laser Module which can be used to synchronize the strobe flash to a remote target or used as a laser tachometer to determine the speed of rotating objects (Tach Mode). The features of the Nova-Pro are highlighted in Figure 1 and Table 1.

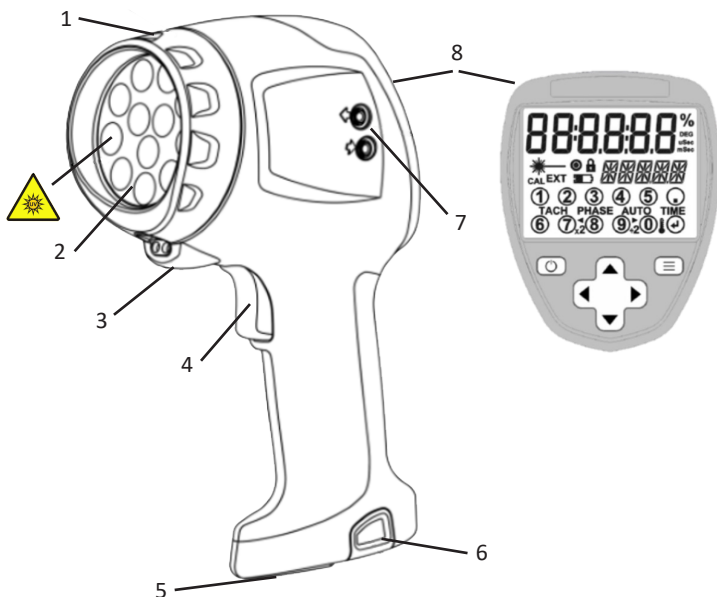


Figure 1 Nova-Pro UV Features

Table 1 Nova-Pro UV Features

1, 2	Bezel and Lens	Bezel is removable to add or remove the Laser Module. UV Emitted from here!
3	Laser Module	Internal laser used to synch the flash to an external marker on the object under inspection; can also be used in Tachometer Mode (patented technology)
4	Trigger	Used to activate the unit (when power is on)
5	Tripod Mount	1/4-20 tripod mount for hands-free operation
6	Power Source	Battery Pack—Removable battery pack; recharged in the external battery Charger Base or AC Power — Plug in for continuous use
7	Input/Output Jacks	Input jack for external trigger devices Output jack for pulse sync for other strobes or data systems
8	User Interface	• Dedicated keypad with “joystick” button for adjusting flash rate • Backlit LCD (Liquid Crystal Display) • Touchscreen keypad for precise flash rate value entry

2.0 USER INTERFACE

The Nova-Pro UV user interface consists of a large backlit display with touch keypad, dedicated keys on the user interface panel, and a trigger to activate the unit when the power is on. The user interface is described in Figure 2 and Table 2.

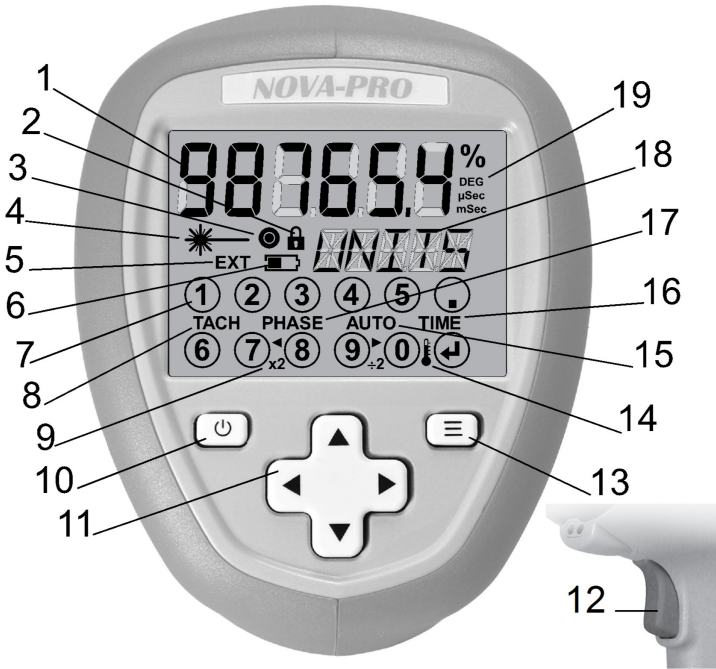


Figure 2 Nova-Pro UV User Interface

Table 2 Nova-Pro UV User Interface

1	6-digit display used to display flash rate and other numeric values
2	Lock icon—active when the device is locked on
3	On-Target indicator—active when the input/laser is locked on to a target; also used to indicate current selection in the menus
4	Laser icon—indicates that the laser is armed (flashing) or on (solid)
5	EXT icon—active when an external source is plugged into the unit
6	Battery icon—active when the battery is low
7	Touch Keypad—(numeric) used to directly enter precise flash rates
8	TACH icon—active when Tachometer Mode is selected
9	x2, ÷2 and arrows—used to double or halve the flash rate
10	POWER button—turns the unit on/off; used as escape/back button in menus and trigger lock
11	Joystick—adjusts flash rate; also used for menu navigation
12	Trigger—used to activate the unit when the power is on
13	MENU button—allows access to the menus; also used to confirm selections
14	Temperature icon—active when the system is overheated
15	AUTO icon—active when unit is in virtual slow motion AUTO VRPM mode
16	TIME icon—active when a TIME DELAY is selected
17	PHASE icon—active when a PHASE DELAY is selected
18	5-digit alphanumeric display used to display units and other statuses
19	Engineering units used in menu for brightness and delay parameters

3.0 GETTING STARTED

3.1 Power

The battery powered Nova-Pro UV has a removable Battery Pack that should be charged before use (see [8.0 BATTERY PACK](#)). The Battery Pack is keyed to ensure correct insertion into the Nova-Pro and Battery Charger. **Make sure to remove the tape protecting the battery terminals and charge the battery before use.**



The AC powered Nova-Pro UV has an external power adapter that must be plugged into an AC outlet (100-240 Vac) using the appropriate connector. Interchangeable plugs allow for operation in most countries ([10.0 WALL POWER SUPPLIES](#)).



With the power source (battery or AC) inserted into the Nova-Pro, turn the unit on by pressing and holding the POWER button until the display illuminates, then release the button. To operate the unit, pull the trigger. The unit will remember the last mode used.

To turn the unit off press and hold the POWER button until the display shows OFF and then release. The unit will also automatically power off after 3 minutes.

3.1.1 Continuous Operation

The unit can be locked in continuous operation by pressing the POWER button while squeezing the trigger. Keep holding the POWER button as you release the trigger and the Lock icon will  show on the display. To remove the lock simply pull the trigger.

3.2 Input/Output Connections

The Nova-Pro UV has input and output jacks on the side that can be used for external triggering or synchronization (daisy chaining two or more strobes). These jacks accept 1/8" [3.5 mm] phone plugs (input-stereo, output-mono). The input jack provides a source of power (5 Vdc @ 75mA) to power an external sensor and will accept a signal from 3 to 12 volts. The output is TTL compatible (3V) and provides a pulse synchronized to the internal generator (flash rate) or external input signal. Connection details are shown in Figures 3 and 4 (below).

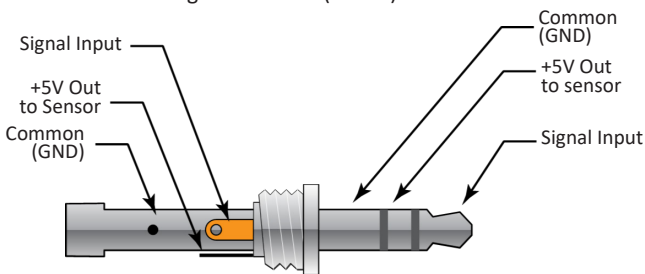


Figure 3 Input Connector Detail (stereo plug)

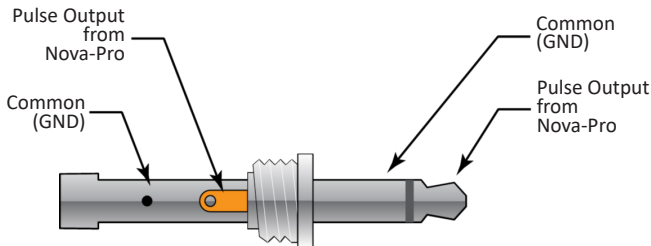


Figure 4 Output Connector Detail (mono plug)

4.0 MODES OF OPERATION


The Nova-Pro UV has four modes of operation: **STROBE**, **LAMP**, **LASER** and **TACH** (Tachometer). The mode can be changed in the Mode Menu (see [5.2 MODE Menu](#)). Each are described in the sections below:

4.1 STROBE Mode

In this mode the strobe generates the flash rate from an internal generator set by the user. The strobe will not flash until the trigger is depressed. The strobe will output a pulse signal from the output jack at the rate of the internal setting whether the trigger is pressed or not. The user can set the flash rate using several methods.

4.1.1 Joystick


Pressing any button on the joystick will cause a digit on the display to start blinking—this is the digit that will be edited. There is a rollover effect when the digit is changed—if incrementing the units digit 99 will roll over to 100. If the user does not increment or decrement a digit within 5 seconds the edit mode will be canceled.



Press ◀ or ▶ to change the digit that blinks.



Press ▲ or ▼ to increase or decrease the value of the blinking digit. Hold for auto increment or decrement.




4.1.2 Touch Keypad Entry

Press the MENU button to display the numeric keypad. The flash rate will default to 0 and show the units you are entering. Note that this is a capacitive touch sensitive keypad and will not respond if the user is wearing gloves.



Press the MENU button.



Enter the desired flash rate and press the enter key ←.

4.1.3 Doubling or Halving the Flash Rate

Press the MENU button twice to display the x2 and ÷2 icons. Press the POWER button to exit this mode.



Press the MENU button twice.



Use the joystick or touch icons on display to x2 or ÷2.

To confirm that the strobe is flashing at the same rate that the target is moving and that the RPM/RPS reading is accurate, use the x2 button until you see a double or multiple image, then use the ÷2 button until you see a single image. This will now be the correct speed as shown in Figure 5 (next page).

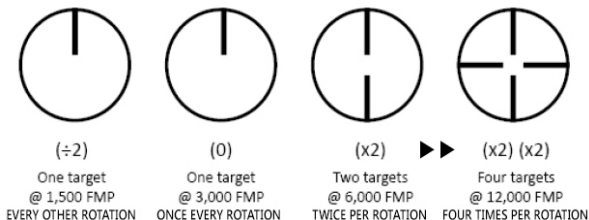


Figure 5 Object rotating at 3000 RPM

NOTE: If doubling or halving the flash rate causes the strobe to exceed its range, the display flash rate will remain at the current flash value.

4.1.4 External Input

Whenever an external source (sensor, signal generator or another strobe) is plugged into the input jack (➡ pointing towards jack) and the unit is in Strobe Mode, the signal from the external source becomes the source of trigger for the flash. The user cannot make any flash rate adjustments and the display will show the rate of the external input.

EXT External icon will show in display when there is an external sensor plugged into the strobe.

Activating the trigger with a valid external input will cause the strobe to flash. If the external input is an optical sensor, activating the trigger will power the sensor. Aim the sensor at the target. Once the strobe has detected the target via the sensor on the rotating or reciprocating machine, the strobe will flash each time a signal is received allowing the user to virtually “stop motion”. The speed read by the external sensor will be shown in the selected units on the display. The strobe can be configured to trigger on the positive or negative edge of the incoming pulse (MENU-MISC).

- On-Target icon will show on the display when a valid external signal is detected.

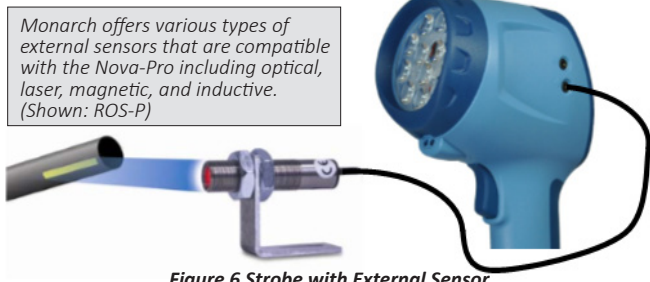


Figure 6 Strobe with External Sensor

4.2 LAMP Mode

For full time activation of the UV light source, the Nova-Pro UV365/UV385 has a Lamp Mode that creates a bright, constant light for inspection. Be aware that this mode uses considerably more battery power and that you should never look directly into the light source. The Nova-Pro UV has a temperature monitor for the LED lights, and will dim the lights if they become overheated during extended use. A thermometer will appear on the display when this happens, and the Nova-Pro may go into shut-down mode if the LEDs get too hot.

4.3 LASER Mode

The Laser Mode is only available when the Laser Module is installed. This mode uses the LASER to trigger the strobe flash and is similar to the External Input Mode.



Laser icon will blink when Laser Mode is enabled and be on solid when trigger is pulled and laser is on.

By pulling the trigger and aiming the laser at a reflective target on the rotating or reciprocating machine, the strobe will flash each time a reflection is received allowing the user to virtually stop motion.

- On-Target icon will show on the display when target is detected by laser.

The flash rate (speed) will be displayed in the selected units.



CAUTION

- **AVOID EXPOSURE—LASER RADIATION IS EMITTED FROM THIS APERTURE**
- **DO NOT STARE DIRECTLY AT THE LASER SOURCE**
- **NEVER VIEW THROUGH OPTICAL INSTRUMENTS**
- **DO NOT AIM AT AIRCRAFT**

Figure 7 Using the Laser Module

4.4 TACH (Tachometer) Mode

The TACH (Tachometer) Mode requires the Laser Module to be installed OR an external input (sensor) be plugged in. This mode uses the laser or external signal to measure rotational speed.

TACH Tachometer icon will show on the display when the Nova-Pro is in TACH Mode.

NOTE: Unit will NOT FLASH in Tachometer Mode.



Laser icon will blink when Laser Mode is enabled and be on solid when trigger is pulled and laser is on.

EXT External icon will show on the display when there is an external sensor plugged into the Nova-Pro.

Pull the trigger and aim the laser (or external sensor) at a reflective target. The speed will be shown in the selected units on the display.





On-Target icon will show on the display when target is detected.

The TACH can be configured to trigger on the positive or negative edge of the incoming pulse from the external input (MENU-MISC).


Refer to Figure 7 (previous page) and associated warnings.

5.0 MENUS

The menu that shows is dependent on the current operating mode of the unit and whether the Laser Module is installed.

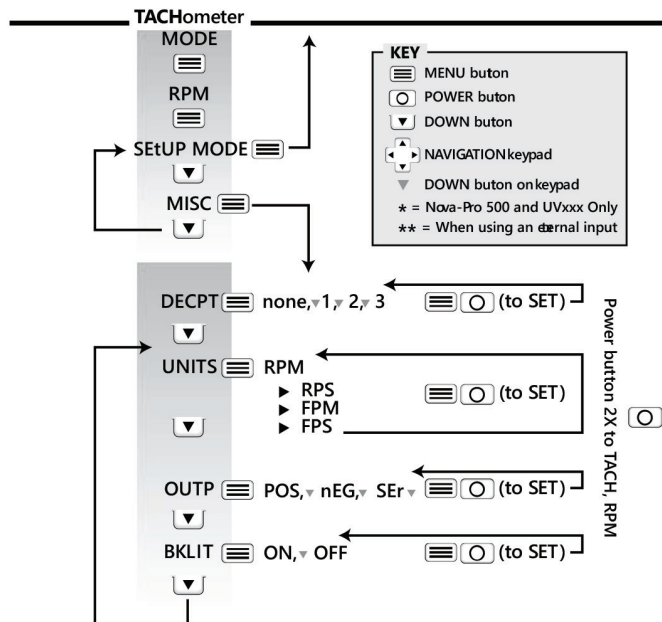

- UP ARROW (▲) will reverse direction through menu
- MENU button (≡) at any menu item will enter that item sub-menu
- POWER button (⏻) will exit the current menu item

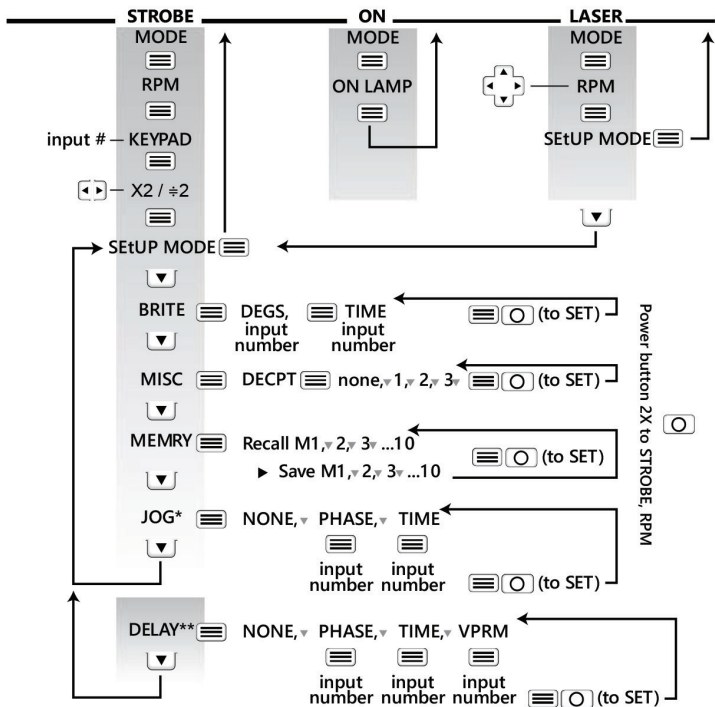

5.1 Menu Overview

To enter the menus, press the MENU button (three-line icon) once or three times depending on the current mode (see Menu Overview) until the word **SETUP** appears on the top line of the display. To select the current item shown on the lower line, press the MENU button again. Not all items will be available in the menu; it depends on the operating mode.

Once in the Setup menu:



Use the ▲ and ▼ arrows on the joystick to scroll through the different available menu options.



Press the MENU button to enter menu options and make selections.



Press the POWER button to escape or back out of the menus.



On-Target icon will show which menu option is selected.

The following sections describe the individual submenus.

5.2 MODE Menu

MODE choices are: **StrobE**, **On** (Lamp), **tACH** (Tachometer), or **LASER** (if Laser Module installed).

Press the MENU  button to enter the MODE menu. The top line will show the mode and the On-Target  indicator will be on for the currently selected mode.



Use the ▲ and ▼ arrows on the joystick to select the desired mode.



Press the MENU button to select the desired mode. This will change the mode and exit the menu.



Press the POWER button to escape without changing the mode.

5.3 Brightness (BRITE) Menu

Refer to [6.0 STROBE BRIGHTNESS](#) for details on Brightness and Flash Duration before using this feature.

The Brightness (BRITE) menu option sets the flash duration which affects the brightness. Flash duration can be adjusted in degrees of rotation (proportional flash duration—changes with flash rate) or time in milliseconds (msec—fixed flash duration). The flash duration will be set by the last flash duration value adjusted. If you adjusted degrees, the strobe will have a flash duration in degrees proportional to the flash rate. If the adjustment was in time, the strobe will have a fixed duration irrespective of the flash rate.

This is a live adjustment—if the trigger is depressed, the effect of changing the brightness can be seen immediately.

5.3.1 Degrees

Press the MENU button  to enter the BRITE menu. The current flash duration will be shown in degrees.

 Use the arrows on the joystick to adjust the flash duration in degrees (refer to [4.1.1 Joystick](#)). Degrees can be set from 0.1° to 10°.

Press the MENU button  followed by the Power button  to save the degree setting.

5.3.2 Time

To set the flash duration in time instead of degrees, press the MENU button  again (skip the DEG menu).

 Use the arrows on the joystick to adjust the time value. Time can be set from 0.001 msec to 2.000 msec.

Press the MENU button  followed by the Power button  to save the time setting.

5.4 Miscellaneous (MISC) Menu

This menu item contains seldom used options. The miscellaneous items are: DECPT (Decimal Point), UNITS, INPUT, OUTP (Output) and BKLIT (Backlight).

Press the MENU button to enter the MISC menu.

Use the ▲ and ▼ arrows on the joystick to scroll through the miscellaneous options.

Press the MENU button to select the desired option.

Press the POWER button to exit/escape.

5.4.1 DECPT (Decimal Point) Menu

The Decimal Point menu adjusts the resolution of the Flash/Tach rate displayed. Up to three places after the decimal point can be shown. The number of decimal places is limited by the 6-digits available and the unit will auto range to show the maximum number of digits after the decimal point selected by the user. The choices are NONE, 1, 2, 3. A value of 600 will be displayed as 600, 600.0, 600.00, 600.000 depending on the setting.

Press the MENU button to enter the DECPT menu. The current value is shown on the top line with DECPT on the lower line. The On-Target indicator will be on for the currently selected value.

Use the arrows on the joystick to select the desired value.

Press the MENU button followed by the Power button to save the decimal point setting.

To exit without setting the decimal point, press the Power button.

5.4.2 UNITS Menu

This menu option selects the Engineering Units used to display the flash rate or speed. The choices are:

FPM Flashes per Minute (not available in TACH Mode)

FPS Flashes per Second (same as Hz; not available in TACH Mode)

RPM Revolutions per Minute

RPS Revolutions per Second (same as Hz)

Press the MENU button to enter the UNITS menu. Unit is shown on the top line with the current engineering unit on the lower line. The On-Target indicator will be on for the currently selected value.

Use the arrows on the joystick to select the desired value.

Press the MENU button followed by the Power button to save the value.

To exit without setting the units, press the Power button.

5.4.3 INPUT Menu

This menu sets the pulse polarity of the external signal that will trigger the strobe. The options are **nEG** for negative edge or **POS** for positive edge.

Press the MENU button to enter the INPUT menu. The current edge setting is shown on the top line with INPUT on the lower line. The On-Target indicator will be on for the currently selected value.

Use the arrows on the joystick to select the desired value.

Press the MENU button followed by the Power button to save the value.

To exit without changing the polarity, press the Power button.

5.4.4 OUTP (OUTPUT) Menu

This menu sets the pulse polarity of the output signal that will trigger a device connected to the output jack. The options are **nEG** for negative pulse or **POS** for positive pulse.

Press the MENU button to enter the OUTPUT menu. The current edge setting is shown on the top line with OUTP on the lower line. The On-Target indicator will be on for the currently selected value.

Use the arrows on the joystick to select the desired value.

Press the MENU button followed by the Power button to save the value.

To exit without changing the polarity press the Power button.

5.4.5 BKLIT (Backlight) Menu

This menu option turns the backlight of the display ON or OFF.

Press the MENU button to enter the Backlight menu.

Use the arrows on the joystick to select the desired value. The backlight will change in real time.

Press the MENU button followed by the Power button to save the value.

To exit without changing press the Power button.

5.5 Memory (MEMRY) Menu

The Memory (MEMRY) menu is used to store (save) or recall up to 10 different strobe settings. The settings that are saved and recalled are the flash rate, brightness and JOG settings (PHASE and TIME). All other settings on the unit remain the same.

Press the MENU button to enter the MEMRY menu.

Use the right arrow ► on the joystick to toggle between SM (Save Memory) or RM (Recall Memory).

5.5.1 Save Memory

To STORE the current strobe setting into a memory location:

Once in the Memory (MEMRY) menu, press the ► arrow on the joystick to enter the Save Mode indicated by SM on the display. Use the ▲ and ▼ arrows on the joystick to select one of the memory locations in which to save the settings—SM1, SM2... SM10.

Press the MENU button followed by the Power button to save the current strobe setting into the displayed location. The current flash rate will then be shown in that location.

To exit without saving a value press the POWER button.

5.5.2 Recall Memory

To RECALL a saved strobe setting:

Once in the Memory (MEMRY) menu, make sure the you are in the Recall Mode as indicated by RM on the display. Use the ▲ and ▼ arrows on the joystick to select one of the memory locations from which to load the settings—RM1, RM2...RM10.

Press the MENU button followed by the Power button to recall the setting from the selected location.

To exit without recalling a memory location press the Power button.

5.6 JOG Menu

This menu option is only valid in the **STROBE Mode** with **NO External Input**. Refer to [7.0 STROBE DELAY](#) for details on DELAY before using this menu item. All delays are relative to the current flash rate.

Press the MENU button to enter the JOG menu. The current setting will be shown and the On-Target indicator will be on for the currently selected value.

Use the arrows on the joystick to select the desired Jog method. The options are: NONE, PHASE, and TIME.

Press the MENU button to select a Jog method. This will enter the sub-menu for PHASE or TIME.

5.6.1 NONE

To cancel the JOG mode, press the MENU button when NONE is displayed.

5.6.2 PHASE

To Jog by PHASE, press the MENU button when PHASE is displayed.

The phase value will be shown in degrees. Use the joystick to set the desired value (refer to [4.1.1 Joystick](#)). Phase can be set from -360.0° to +345.0°.

Press the MENU button to accept and exit.

5.6.3 TIME

To Jog by TIME, press the MENU button when TIME is displayed.

The time value will be shown in milliseconds. Use the joystick to set the desired value (refer to [4.1.1 Joystick](#)). Time can be set from -50.000 msec to +50.000 msec.

Press the MENU button to accept and exit.

To exit the JOG Menu, press the Power button.

NOTE: Once a setting has been selected using PHASE and TIME in the JOG menu, that setting will persist even through a power cycle.

The PHASE/TIME icon will be illuminated on the display to let the user know that the delay is being applied to the flash setting. To remove the setting, navigate to the JOG menu and use the joystick to select NONE. Multiple PHASE or TIME settings can also be added as a parameter in any of the 10 MEMORY locations. (Refer to [5.5 Memory Menu](#).)

5.7 DELAY Menu

This menu option is only valid in the **STROBE Mode** with an **External Input** or in the **Laser Mode**. Refer to [7.0 STROBE DELAY](#) for details on DELAY before using this menu item. All delays are relative to an external trigger which may be derived from the internal laser or external input.

Press the MENU button to enter the DELAY menu. The current setting will be shown and the On-Target indicator will be on for the currently selected value.

Use the arrows on the joystick to select the desired Delay method. The options are: NONE, PHASE, TIME and VRPM.

Press the MENU button to select a Delay method. This will enter the sub-menu for PHASE, TIME or VRPM.

5.7.1 NONE

To cancel the DELAY mode, press the MENU button when NONE is displayed.

5.7.2 PHASE

To Delay by PHASE, press the MENU button when PHASE is displayed.

This method of delay is set the same as PHASE in JOG.

NOTE: The adjustments happen in **real time**, so if the strobe is flashing the user can view the effect of changing the delay.

5.7.3 TIME

To Delay by TIME, press the MENU button when TIME is displayed.

This method of delay is set the same as TIME in JOG.

NOTE: The adjustments happen in **real time**, so if the strobe is flashing the user can view the effect of changing the delay.

5.7.4 VRPM

Virtual RPM (VRPM) is an AUTO delay mode. To set VRPM, press the MENU button when VRPM is displayed.

The virtual RPM value will be shown. Use the joystick to set the desired value (refer to [4.1.1 Joystick](#)). VRPM can be set from -60.0 RPM to +60.0 RPM.

Press the MENU button to accept and exit.

NOTE: The adjustments happen in **real time**, so if the strobe is flashing the user can view the effect of changing the RPM.

To exit the DELAY Menu, press the Power button.

Press the Power button to escape back out of the setup menu.


6.0 STROBE BRIGHTNESS

The strobe's brightness depends on how wide the strobe's flash pulse is; the wider the pulse, the brighter the flash from the LEDs appears to be. However, there is a downside to the wider pulses. All strobes work by giving short bursts of light (the pulse width) at a rapid repetition rate (the flash rate). Strobes rely on the persistence of the human eye (the ability to remember an image) and its response to bright light to give an apparent stop motion image. Imagine a shaft rotating at 6000 RPM or one rotation every $1/100$ of a second (10 msec). If the strobe flashes once every 10 msec for a brief moment, the user sees the flash at the same spot in the rotation of the shaft and the persistence of the eye remembers this until the next flash making the shaft appear to be stopped. As the target is rotating there is some movement evident during the strobe flash. The longer the flash duration, the more obvious the rotation is and this increases the blur.

6.1 Calculating Blur

Blur can be calculated – if the shaft is turning at 6000 RPM, it takes 10 msec to complete one revolution. If the strobe flash duration is 100 μ sec ($1/100$ of a millisecond), the shaft will turn: $(\text{flash duration}/\text{time per rotation}) \times 360^\circ$, which is $(.0001/.01) \times 360 = 3.6^\circ$. So you will see the shaft appear to move 3.6° .

As the flash pulse widens you will see greater degrees of rotation which results in more blur and a brighter perceived illumination (the LEDs are on longer so the average light the eyes see is greater). The trade off is blur versus brightness. The further away the rotating point is from the center axis the faster the tangential velocity and the worse the blur appears to be.

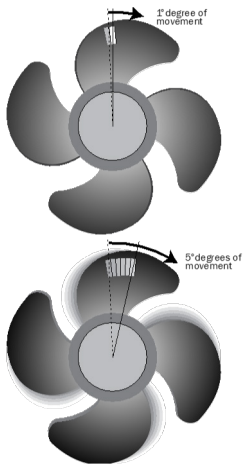

When setting the pulse duration in degrees, what you set is what you get. Refer to the image on the previous page for the difference between a 1° and 5° (of rotation) flash duration.

There are two methods of adjusting the flash pulse width and hence the brightness and consequently the blur. For setting brightness, see [5.3 Brightness \(BRITE\) Menu](#).

6.2 Brightness in Degrees of Rotation

Brightness can be set from 0.1 to 10 degrees out of 360. The higher the setting the brighter the strobe appears to be but the more blurred the target is. Optimal setting to stop motion is 1.8 to 3.6°. The number of degrees is a proportional amount and remains constant as the flash rate increases or decreases. The strobe automatically calculates how wide the pulse width should be at different flash rates to keep the blur constant—the faster the flash rate the narrower the pulse width. The pulse width equals: (setting in degrees/360) x (1/flash rate in Hz).

6.3 Brightness in Pulse Duration

Brightness can also be set to a fixed duration pulse in milliseconds. The flash rate remains constant irrespective of the flash rate, thus as the flash rate increases, the image will get brighter and more blurred.

NOTE: There are two limits maintained by the strobe – the flash pulse width can never be greater than 2.0 msec (milliseconds) nor can it exceed 10° of rotation.

The strobe automatically adjusts the pulse width and rotation values as the flash rate is increased or decreased to maintain the limits at all times. For example – a flash rate of 600 flashes per minute (10 Hz), 10° of rotation represents a flash pulse width of 2.8 msec. The strobe will limit this value to 2.0 msec or 7.2° of rotation (blur).

7.0 STROBE DELAY

The Nova-Pro UV has multiple special effects that can be used to inspect moving machinery in different ways. The Delay effects depend on whether a Laser Module is installed and the Mode of Operation. Delay, or Phase Shifting, allows the user to view different positions of the rotating machinery relative to a virtual or fixed trigger point (via External sensor or internal Laser).

7.1 Internal Phase Delay (JOG)

In the internal STROBE Mode the Delay is relative and no external trigger is used. This is referred to as JOG. Once the flash rate has been adjusted to give a stopped motion image, the JOG buttons (◀ and ▶ icons on the touchpad) may be used to increase or decrease the phase of the image with respect to its original position by the amount set in the JOG Menu.

Use this feature to bring a reference mark, such as a keyway, into your line of sight. It may be necessary to adjust the flash rate to keep the target static if the speed is drifting.

Use the JOG Menu to set a PHASE Delay of -30° . The **PHASE** display will show PHASE with the left and right arrow ◀ ▶ icons. Use the joystick to adjust the flash rate to stop motion of the rotating object. Then use the ◀ and ▶ icon touch buttons to move the phase of the objects as shown in Figure 8 (below).

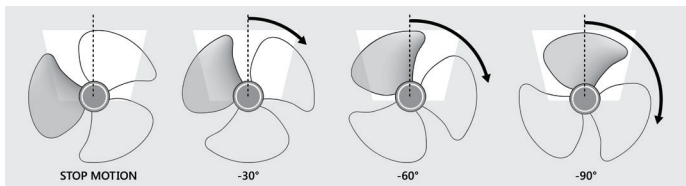


Figure 8 Phase Shifting by -30° , -60° , -90°

7.2 External / Laser Delay

There are three External Delay Modes: **Phase Delay**, **Time Delay** and **Auto (Virtual RPM)**. These modes are only active if an external trigger source is available via the internal Laser Module or an external sensor.

7.2.1 Phase Delay

In the External Phase Delay Mode the flash is delayed from the external trigger by the number of degrees set in the DELAY PHASE menu ($+345.0^\circ$ to -360.0°). One revolution is 360° . The display will show the **PHASE** icon to indicate the delay mode. See Figure 9 (below) for examples of the effect of setting various PHASE delays with respect to the trigger point.

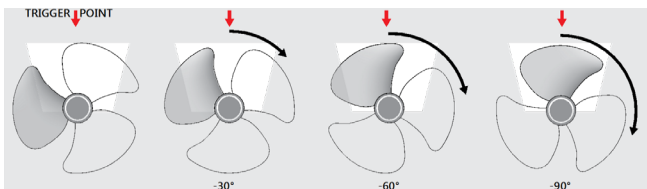


Figure 9 Phase Shifting by -30° , -60° , -90°

The Phase Delay tracks the speed of the target; the strobe is continuously computing the delay angle for the current speed. In the Menu, the adjustments happen in **real time**, so if the strobe is flashing, the user can view the effect of changing the delay.

7.2.2 Time Delay

In the External Time Delay mode the flash is delayed from the external trigger by the time in milliseconds (msec) set in the DELAY TIME menu (-50.000 to +50.000 msec). The TIME Delay is absolute and remains constant irrespective of the speed of the target. The display will show the **TIME** icon to indicate the Delay Mode. The effect is similar to Figure 9 but the delay will be in the millisecond setting in the TIME Menu. In the Menu, the adjustments happen in **real time**, so if the strobe is flashing the user can view the effect of changing the delay.

7.2.3 AUTO—Virtual RPM

In the AUTO (Virtual RPM—VRPM) mode the flash is automatically delayed in increasing or decreasing amounts after the external trigger pulse so that the image appears to rotate at a slow speed (Virtual RPM) as set in the VRPM menu (0 to 60 RPM). This gives a “slow-motion” effect and enables the target to be examined as it moves through a complete cycle or revolution. The display will show the **AUTO** icon to indicate the Delay Mode with the virtual speed in RPM on the top line and will indicate VRPM (Virtual RPM) on the lower line. In the Menu, the adjustments happen in **real time**, so if the strobe is flashing the user can view the effect of changing the virtual RPM.

NOTE: Turning the power off will reset the delay modes.

8.0 BATTERY PACK

The Nova-Pro UV comes with one rechargeable Lithium-ion battery pack and external charging station with associated power supply. The Battery Pack is shipped in a mostly discharged state and has tape over the terminals.



CAUTION:

- Do not store battery in hot locations
- Do not expose to fire
- Do not disassemble
- Do not apply mechanical force
- REMOVE Battery Pack from unit before storing for long periods



DO NOT DISPOSE of the lithium-ion batteries as unsorted municipal waste. The batteries need to be **RECYCLED** in accordance with local regulations. The batteries should be sent to a recycling center or returned to the factory using appropriate shipping methods.



The Nova-Pro Battery Pack is specifically keyed to fit in the Nova-Pro unit and Nova-Pro Charging Station one way only. Insert the Battery Pack into the Nova-Pro until the clips lock into place. To remove, squeeze clips on the Battery Pack to release from the Nova-Pro. The Battery Pack can also be screwed into the Nova-Pro using the attached captive screw.

8.1 Low Battery Functionality



Low battery icon will blink when battery pack needs to be recharged. The unit may still be used for a short time.

The Nova-Pro will display LOBAT and shut down when the battery pack is exhausted and must be recharged.


8.2 Charging the Battery Pack

The Nova-Pro Battery Pack must be removed from the Nova-Pro unit to be charged using the Nova-Pro Charging Station (shown right) and power supply provided (see [10.0 WALL POWER SUPPLIES](#)).



CAUTION:

Never attempt to charge the Battery Pack with anything other than the Charging Station and power supply provided with the Nova-Pro.



The Nova-Pro Charging Stations has a light emitting diode (LED) that indicates the state of the battery/station The LED indicates the following:

- Green = On / No Battery or Battery Charged
- Red = Charging
- Flashing Red = Error / Replace Battery

Battery charge time will be up to 6 hours depending on Battery Pack and residual charge. Once the battery is charged the charger will switch to trickle charge mode—the battery should be removed once the charge LED turns green.

9.0 OPTIONAL AC POWER

An optional AC Power Adapter can be ordered to convert the Nova-Pro UV from a battery-powered unit to AC powered allowing for continuous operation from AC power. Simply insert the AC Power Adapter into the Nova-Pro (matching the keyed slot) until it clicks into place and use the captive screw to secure it into place. Then plug the wall power supply into an outlet (100 Vac to 240 Vac) using the appropriate interchangeable plug.



10.0 WALL POWER SUPPLIES

The wall power supply provided with the Nova-Pro Charging Station and optional AC Power Adapter has interchangeable plugs allowing it to be used with AC outlets in different countries.



To change the plugs, depress the button on the installed plug and slide the plug up and out of the power supply. Select the correct plug and slide it back into the power supply until the plug seats firmly. Make sure the plug cannot slide out.

CAUTION: RISK OF ELECTRIC SHOCK

- Do not insert the plugs into an AC outlet without the power supply attached
- Avoid touching the plug blades when inserting or removing the power supply from the AC outlet
- Indoor use only



11.0 SPECIFICATIONS

Specifications*	Nova-Pro® Ultraviolet UV365 & UV385 Stroboscopes
Flash Range	30 to 999,999 FPM/RPM
Display	6-digit numeric and 5-digit alphanumeric LCD with touch keypad; high contrast blue background/white characters with backlight
Accuracy	0.001% of setting ± 1 lsd
Resolution	6 digits to 0.001
Light Source	UV365 nm or UV385 nm 12 LED Array
Light Output	1700 $\mu\text{W}/\text{cm}^2$ @ 12", 1% duty cycle
Flash Duration	Adjustable to 10°/2.000 msec max
External Triggers Input/Output	TTL (12 Vdc) max input; provides 3.3 Vdc TTL output
Programmable Memory	10 setpoints
Internal Phase Shift	Yes
Phase Delay	-360.0 to 345.0 degrees
Time Delay	-50.000 to 50.000 msec
Virtual RPM - Slow Motion	-60.00 to 60.00 VRPM
Operating Time	Battery Pack: 9.5 hours typical (6000 FPM, 2° duty cycle)
Power Supply - Battery	Removable/rechargeable Li-ion battery pack with 100-240 50/60 Hz recharging station Battery: 7.4V, 2.8Ah (21W)

Specifications*	Nova-Pro® Ultraviolet UV365 & UV385 Stroboscopes
Power Supply - AC	100-240 Vac 50/60Hz AC adapter with 6 ft. [2 m] cable and interchangeable outlet adapters (optional)
Weight	1.4 lbs. [635 g] with battery
Size (HxWxD)	9.5 x 3.75 x 5.5 in. [241 x 95 x 140 mm]
Housing Material/ Rating	ABS/IP54

*Specifications are subject to change without notice.

11.1 Operating Environment

This equipment is NOT intended for permanent installation.
This equipment is for use in a controlled environment—Environmental situation A, Pollution Degree 2.

Altitude: up to 2000 m

Temperature: 5°C to 40°C

NOTE: The Temperature icon will turn on if the LED array exceeds 75°C and the unit will reduce flash duration to lower temperature.
The unit will shut off if the temperature exceeds 85°C.

Humidity: Maximum relative humidity 80% for temperatures up to 31°C decreasing linearly to 50% relative humidity at 40°C

Rating: IP54 (splash-proof)

Category: 2

11.2 Compliance

11.2.1 Battery Compliance

The Lithium-ion battery packs used in this product meet the requirements of UN DOT 38.3.

Tested by Shenzhen SEM.Test Technology Co. Ltd. (Reports STR16079052S/54S).

11.2.2 EU Declaration of Conformity

Please visit our website www.monarchinstrument.com to download our EU Declaration of Conformity for this product.

11.2.3 Energy Efficiency

This product complies with the U.S. Department of Energy's energy conservation standards specified in the Code of Federal Regulations 10 CFR 430.32(z) and is registered in the DoE CCMS database. (BC)

12.0 ACCESSORIES

There are many accessories available to enhance the functionality and keep your Nova-Pro up and running. See Monarch Instrument's website for detailed information. [Accessories webpage](#).

[See Sensors webpage for more details.](#)

Sensors:

ROLS-P

Remote Optical Laser Sensor w/ 8 ft. [2.5 m] cable

RLS-P

Rugged Laser Sensor w/ removable 9.8 ft. [3 m] cable with watertight M12 connector

ROS-P

Remote Optical Laser Sensor w/ 8 ft. [2.5 m] cable

ROS-P-25

Remote Optical Sensor w/ 25 ft. [7.6 m] cable

IRS-P

Infrared Sensor w/ 8 ft. [2.5 m] cable for use triggering strobe use w/out reflective target at 0.5 in. [2 mm] gap

MT-190P

Magnetic Trigger Sensor/Amplifier w/ 8 ft. [2.5 m] cable



Measure • Monitor • Maintain

Monarch Instrument is committed to excellence and quality in manufacturing, sales, and service.



Portable Tachometers



Track-It™ Data Loggers



Panel Tachometers



Fixed Mounted Strobes



Portable Strobes



Frequency Converters



Speed Sensors



DataChart™ Paperless Recorders



MONARCH
INSTRUMENT

15 Columbia Drive, Amherst NH 03031 USA

Tel.: (603) 883-3390 // (800) 999-3390

Email: support@monarchinstrument.com

Website: www.monarchinstrument.com